Engineering in Medicine

Volume 16 1987

Author Index

Anderson, J. B. A leg positioning and holding mechanism for use during knee surgery, 163
Arokoski, J. Indentation study of the biomechanical properties of articular cartilage in the canine knee, 15
Atkinson, J. R. The causes of femoral head roughening in explanted Charnley hip prostheses, 167

Bilton, G. The in vivo durability of bioprosthetic heart valves – modes of failure observed in explanted valves, 95
Bird, H. A. A review of some of the rheumatological problems and engineering capabilities, 191
Black M. M.
Artificial heart valves — past, present, and future, 61
The long-term clinical assessment of heart valve substitutes, 87
The in vivo durability of bioprosthetic heart valves – modes of failure observed in explanted values, 95
Bowker, P. The role of gait analysis in clinical medicine: a survey of UK centres, 221
Broek, J. S. Body surface measurement and replication by photogrammetry and computer aided design, 3
Burton, A. K. The ratio of upper lumbar to lower lumbar sagittal mobility related to age, sex, and low back trouble, 233

Calderale, P. M.
Mathematical models of musculo skeletal systems, 131
A mathematical model of the locomotor apparatus, 147
Cathcart, L. Laboratory assessment of the design, function, and durability of pericardial bioprostheses, 105
Chamberlain, M. A. Assessment of a new hip dynamometer, 213
Churches, A. E. A leg positioning and holding mechanism for use during knee surgery, 163
Cox, A. J. An automated technique for in vitro assessment of the susceptibility of urinary catheter materials to encrustation, 37
Crofts, C. E. Pericardial heterografts: a method of leaflet mechanical property control, 111
Cunningham, J. L. The measurement of stiffness of fractures treated with external fixation, 229
Cutts, A. An in vitro method for the measurement of sarcomere length in human muscle, 195

Davies, K. E. An automated technique for in vitro assessment of the susceptibility of urinary catheter materials to encrustation, 37
Dowson, D. The causes of femoral head roughening in explanted Charnley hip prostheses, 167
Drury, P. J.
The long-term clinical assessment of heart valve substitutes, 87
The in vivo durability of bioprosthetic heart valves – modes of failure observed in explanted valves, 95

Ellis, M.
Assessment of a new hip dynamometer, 213
A clinical gait analysis system, 217
Evans, M. The measurement of stiffness of fractures treated with external fixation, 229

Fisher, J. Laboratory assessment of the design, function, and durability of pericardial bioprostheses, 105
Fisher, W. E. A leg positioning and holding mechanism for use during knee surgery, 163
Fraser, S. M. Microwave thermography in rheumatic disease, 209

Gentle, C. R. The use of ceramics in prosthetic heart valves, 115
Giersiepen, M. Laboratory testing of prosthetic heart valves, 67
Gola, M. M. Some experimental results concerning the mechanical coupling in endoprosthetics, 23
Green, J. Assessment of a new hip dynamometer, 213
Gugliotta, A. Some experimental results concerning the mechanical coupling in endoprosthetics, 23

Harris, J. D. The measurement of stiffness of fractures treated using external fixation, 229
Heiliger, R. Hydrodynamic advantages and disadvantages of mechanical bileaflet valves and tilting disc valves No. 29, 77
Helliwell, P. S.
The measurement of stiffness in the rheumatoid hand, 203
Assessment of a new hip dynamometer, 213
Helminen, H. J. Indentation study of the biomechanical properties of articular cartilage in the canine knee, 15
Howe, A.
The measurement of stiffness in the rheumatoid hand, 203
Assessment of a new hip dynamometer, 213
A clinical gait analysis system, 217
Hukins, D. W. L. An automated technique for in vitro assessment of the susceptibility of urinary catheter materials to encrustation, 37

Irlam, J. C. An automated technique for in vitro assessment of the susceptibility of urinary catheter materials to encrustation, 37
Isaac, G. H. The causes of femoral head roughening in explanted Charnley hip prostheses, 167

Jack, G. R. Laboratory assessment of the design, function, and durability of pericardial heterografts, 105
Jurvelin, J. Indentation study of the biomechanical properties of articular cartilage in the canine knee, 15

Kay, R. The long-term clinical assessment of heart valve substitutes, 87
Kennedy, P. D. The causes of femoral head roughening in explanted Charnley hip prostheses, 167
Kenwright, J. The measurement of stiffness of fractures treated with external fixation, 229
Kesavan, S. K. Perspectives in non-traditional biofluid mechanics, 43
Khodadadeh, S.
Quantitative approach to osteoarthritis gait assessment, 9
Force plate studies of Duchenne muscular dystrophy, 177
Kiviranta, I. Indentation studies of the biomechanical properties of articular cartilage in the canine knee, 15
Knott, E. Laboratory testing of prosthetic heart valves, 67

Land, D. V. Microwave thermography in rheumatic disease, 209
Lawford, P. V.
The long-term clinical assessment of heart valve substitutes, 87
The in vivo durability of bioprosthetic heart valves – modes of failure observed in explanted values, 95

© MEP Ltd 1988 Vol. 17 No. 2

Lord, M. Curve and surface representation by iterative B-spline fit to a data point, 29

McClelland, M. Force plate studies of Duchenne muscular dystrophy, 177
McKenna, F. Assessment of a new hip dynamometer, 213
Messenger, N. The role of gait analysis in clinical medicine: a survey of UK centres, 221

Patrick, J. H. Force plate studies of Duchenne muscular dystrophy, 177

Ranu, H. S. The thermal properties of human cortical bone: an in vitro study, 175
Reddy, N. P. Perspectives in non-traditional biofluid mechanics, 43
Reece, I. J. Laboratory assessment of the design, function, and durability of pericardial bioprostheses, 105
Reul, H. Laboratory testing of prosthetic heart valves, 67
Roberts, K. The in vivo durability of bioprosthetic heart valves – modes of failure observed in explanted valves, 95

Scelfo, G.
Mathematical models of musculo skeletal systems, 131
A mathematical model of the locomotor apparatus, 147
Smeathers, J. E. Measurement of flexural and torsional stiffness for the human torso in vivo; implications for scoliosis, 237
Smith, M. R. The causes of femoral head roughening in explanted Charnley hip prostheses, 167
Sturrock, R. D. Microwave thermography in rheumatic disease, 209
Sutton, T. M. An automated technique for in vitro assessment of the susceptibility of urinary catheter materials to encrustation, 37

Tammi, M. Indentation study of the biomechanical properties of articular cartilage in the canine knee, 15
Taylor, K. M. Clinical aspects of heart valve replacement: an overview, 63
Trowbridge, E. A. Pericardial heterografts: a method of leaflet mechanical property control, 111

Van Voorden, A. Body surface measurement and replication by photogrammetry and computer aided design, 3
Vergeest, J. S. M. Body surface measurement and replication by photogrammetry and computer aided design, 3

Walsh, M. J. A leg positioning and holding mechanism for use during knee surgery, 163
Wheatley, D. J. Laboratory assessment of the design, function, and durability of pericardial bioprostheses, 105
Wheble, V. H. Ambulance transport: a question of patient comfort, 47
Wright, V.
Measurement – clinical needs and engineering possibilities (Conference Report), 189
The measurement of stiffness in the rheumatoid hand, 203

Subject Index

Titles of papers are shown in bold type

A clinical gait analysis system, 217
A leg positioning and holding mechanism for use during knee surgery, 163
A mathematical model of the locomotor apparatus, 147
A review of some of the rheumatological problems and engineering capabilities, 191
Ambulance transport: a question of patient comfort, 47
An automatic technique for in vitro assessment of the susceptibility of urinary catheter materials to encrustation, 37
An in vitro method for the measurement of sarcomere length in human muscle, 195
Articular cartilage in the canine knee, biomechanical properties of, 15
Artificial arteries, 246
Artificial hand, 124
Artificial heart valves – past, present, and future, 61
Artificial hip, cementless, 179
Artificial hip joint, 124
Artificial limbs, fatigue testing of, 245
Assessment of a new hip dynamometer, 213
Assessment of osteoarthritic gait, 9
Assessment of the susceptibility of urinary catheter materials to encrustation, 37

B-spline fit, 29
Bileaflet valves, mechanical, 77
Biofeedback postural monitor, 125
Biofluid mechanics, 43
Biological telemetry system, 122
Biomechanical properties of articular cartilage in the canine knee, 15
Bioprostheses, pericardial, 105
Bioprosthetic heart valves, 95
Blood plasma separator, 126
Body scanner, 121
Body surface measurement and replication by photogrammetry and computer aided design, 3
Bone, cortical, 175

Camera laser system, 241
Canine knee, biomechanical properties of articular cartilage in, 15
Catheter, urinary, 37
Cementless artificial hip, 179
Ceramics, 115
Cerebral palsy children:
award scheme for new aid technologies, 120, 181
standing frame for, 122
Charnley hip prostheses, 167
Clinical assessment of heart valve substitutes, 87
Clinical gait analysis, 217
Clinical medicine, role of gait analysis in, 221
'Cold' coagulator, 53
Communicator, synthetic voice, 126
Computer aided design, 3
Computer aided draughting, 179
Contact lens modification unit, 243
Cortical bone, human, 175
Crutches, 180
elbow, 245
Curve and surface representation by iterative B-spline fit to a data point, 29
Defibrillator, 54
Department of Health and Social Security (DHSS), 183
Duchenne muscular dystrophy, 177

Elbow crutches, 245
Electronic podometer, 180
Elevating toilet seat, 243
Encrustation, susceptibility of urinary catheter materials to, 37
Endoprosthetics, 23
External fixation, stiffness of fractures treated with, 229

Femoral head roughening, causes of, 167
Fixation, external, 229
Floating stretcher, 125
Force plate studies of Duchenne muscular dystrophy, 177

Gait analysis, 221
system, 217
Gait assessment, 9

Hand, artificial, 124
Hand, rheumatoid, 203
Hearing aids, 244
Hearing centre, 244
Heart valves, artificial, *see* Heart valve substitutes
Heart valves, prosthetic, *see* Heart valve substitutes
Heart valve replacement, *see* Heart valve substitutes
Heart valve substitutes, 61, 63, 67, 87, 115
Heated mattress, 55
Heterografts, pericardial, 111
Hip, artificial, 124, 179
Hip dynamometer, 213
Hip joint, artificial, *see* Hip, artificial
Hip prostheses, Charnley
Home lifts – safety specification, 51
Human cortical bone, thermal properties of, 175
Human muscle, sarcomere length in, 195
Human torso, flexural and torsional stiffness of, in vivo, 237

Engineering in Medicine © MEP Ltd 1988

Hydrodynamic advantages and disadvantages of mechanical bileaflet valves and tilting disc valves No. 29, 77
Hydrophobic disposable air filter, 54

Indentation study of the biomechanical properties of articular cartilage in the canine knee, 15
Iterative B-spline fit to a data point, 29

Joint replacement design, 179

Knee brace, 243
Knee surgery, 163

Laboratory assessment of the desig.., function, and durability of pericardial bioprostheses, 105
Laboratory testing of prosthetic heart valves, 67
Laser eye surgery, YAG, 52
Leaflet mechanical property control, 111
Leg positioning and holding mechanism, 163
Lens meter, 243
Limbs, artificial, 245
Locomotor apparatus, mathematical model of, 147
Low back trouble, 233
Lumbar mobility, 233

Mathematical model of the locomotor apparatus, 147
Mathematical models of musculo skeletal systems, 131
Measurement – clinical needs and engineering capabilities (Conference Report), 189
Measurement of flexural stiffness for the human torso in vivo: implications for scoliosis, 237
Measurement of stiffness in the rheumatoid hand, 203
Mechanical bileaflet valves, 77
Mechanical coupling, 23
Medic Design Awards, 122
Medical instrumentation, 121
Micro-ophthalmic cannulae, 246
Microwave thermography in rheumatic disease, 209
Model, mathematical, of the locomotor apparatus, 147
Models, mathematical, of musculo skeletal systems, 131
Models of failure of bioprosthetic heart valves, 95

Operating table, 242
Ophthalmic laser, 182
Orthopaedic scooter, 53
Orthotics, 183
Osteoarthritic gait, 9

Multi-sensory stimulation play environment for blind or partially sighted children, 123
Muscular dystrophy, 177
Musculo skeletal systems, 131

National Health Service, 183
Non-traditional biofluid mechanics, 43
North Staffordshire Polytechnic, 184

Patient comfort in ambulance transport, 47
Patient lifter, batter powered, 51
Patient simulators, 121
Pediatric cot, 123
Pericardial bioprostheses, design, function, and durability of, 105
Pericardial heterografts: a method of leaflet mechanical property control, 111
Peristaltic pump tubing, 180
Personal robot, 55
Perspectives in non-traditional biofluid mechanics, 43
Photogrammetry, 3
Podometer, electronic, 180
Postural monitor, 125
Prostheses, hip, 167
Prosthetic heart valves:
laboratory testing of, 67
use of ceramics in, 115

Quantitative approach to osteoarthritic gait assessment, 9
Queens Award for Export Achievement 1987, 246

RADAR (Royal Association for Disability and Rehabilitation), 183
Refractometer, automatic, 244
Rheumatic disease, microwave thermography in, 209
Rheumatoid hand, stiffness in, 203
Rheumatological problems, 191
Roentgen stereophotogrammetric study, 182

Sarcomere length in human muscle, measurement of, 195
Scoliosis, 237
Services for disabled people, 183

Some experimental results concerning the mechanical coupling in endoprosthetics, 23
Specimen mailing packs, 121
Standing frame for cerebral palsy children, 122
Stiffness in the rheumatoid hand, measurement of, 203
Stiffness of fractures treated with external fixation, 229
Stiffness of the human torso, 237
Stretcher, floating, 125
Surface representation, 3
Surgical lasers, 184
Synthetic voice communicator for the disabled, 126

The causes of femoral head roughening in explanted Charnley hip prostheses, 167
The clinical aspects of heart valve replacement: an overview, 63
The in vivo durability of bioprosthetic heart valves – modes of failure observed in explanted valves, 95
The long-term clinical assessment of heart valve substitutes, 87
The measurement of stiffness in the rheumatoid hand, 203
The measurement of stiffness of fractures treated with external fixation, 229
The ratio of upper lumbar to lower lumbar saittal mobility related to age, sex, and low back trouble, 233
The role of gait analysis in clinical medicine: a survey of UK centres, 221
The thermal properties of human cortical bone: an in vitro study, 175
The use of ceramics in prosthetic heart valves, 115
Therapeutic bath, 119
Therapy feedback monitor, 53
Thermal linescan recorder, 183
Tilting disc valves, 77
Traction unit, variable, 55
Tube fittings, 122

Urinary catheter materials, 37

Washing equipment for the disabled and elderly, 119
Wheelchairs, 51, 53, 119, 123
incorporated in therapeutic bath, 119
Whole body monitor, 54
Work-top for the disabled, elderly, or handicapped, 123

YAG laser eye surgery, 52

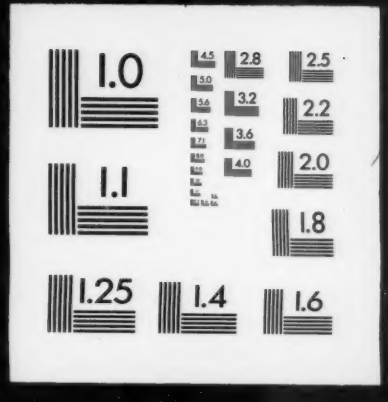
1.0
1.1
1.25
1.4
1.6
1.8
2.0
2.2
2.5
2.8
3.2
3.6
4.0
4.5
5.0
5.6
6.3
7.1
8.0
9.0